

Leptin (Mouse) Enzyme Immunoassay Kit Protocol

(Cat. No.:EK-003-13-B)

(Range: 0.03-300ng/ml)



PHOENIX PHARMACEUTICALS, INC.

INTRODUCTION

This Enzyme Immunoassay kit is designed to detect a specific peptide and its related peptides based on the principle of "competitive" enzyme immunoassay.

PRINCIPLE OF ENZYME IMMUNOASSAY WITH THIS KIT

The immunoplate in this kit is pre-coated with a secondary antibody and the non-specific binding sites are blocked. The secondary antibody can bind to the Fc fragment of the primary antibody (peptide antibody) whose Fab fragment will be competitively bound by both biotinylated peptide and peptide standard or targeted peptide in samples. The biotinylated peptide interacts with streptavidin-horseradish peroxidase (SA-HRP) which catalyzes the substrate solution composed of 3,3',5,5'-tetramethylbenzidine (TMB) and hydrogen peroxide to produce a blue colored solution. The enzyme-substrate reaction is stopped by hydrochloric acid (HCl) and the solution turns yellow. The intensity of the yellow is directly proportional to the amount of biotinylated peptide-SA-HRP complex but inversely proportional to the amount of the peptide in standard solutions or samples. This is due to the competitive binding of the biotinylated peptide with the standard peptide or samples to the peptide antibody (primary antibody). A standard curve of known concentration can be established accordingly. The unknown concentration in samples can be determined by extrapolation to this standard curve.

KIT MATERIALS

1. **20x** assay buffer concentrate (50ml).....**Catalog no. EK-BUF**
2. 96 well immunoplate (1plate).....**Catalog no. EK-Plate**
3. Acetate plate sealer (APS), (3 peices).....**Catalog no. EK-APS**
4. Primary anitbody**Catalog no. EK-RAB-003-13-B**
(rabbit anti-IgG) (1 vial).
5. Standard peptide (1vial).....**Catalog no. EK-S-003-13-B**
6. Positive Control (2 vials).....**Catalog no. EK-PC-003-13-B**
7. Biotinylated peptide (1 vial)..... **Catalog no. EK-B-003-13-B**
8. Streptavidin-horseradish peroxidase..... **Catalog no. EK-HRP**
9. Substrate solution (TMB) (12ml)..... **Catalog no. EK-TMB**
10. 2N HCl (15ml)..... **Catalog no. EK-HCl**
11. Assay diagram (1 sheet).
12. General protocol (1 book).

MATERIALS REQUIRED BUT NOT SUPPLIED

1. Microtiter plate reader capable of absorbance measurement of 450nm.
2. Orbital plate shaker capable of 300-400rpm (Recommended)
3. Microtiter plate washer (Receommended)
4. Multi-channel pipette capable of dispensing 50-100 μ l (Recommended)
5. Solution reservoir (Recommended)
6. Absorbent material for blotting.
7. EDTA Lavender Vacutainer tubes (optional)..**Catalog no. VT-6450**
8. Aprotinin (0.6TIU/ml of blood)(optional)...**Catalog no. RK-APR0**

Phoenix Pharmaceuticals Inc. guarantees that its protducts conform to the information contained in this publication. The purchaser must determine the suitability of the product for its particular use and establish optimum sample concentrations.

NOTE: This kit should be equilibrated to room temperature (20-23°C) before opening any vials and starting the assay. **It is highly recommended that the solutions be used as soon as possible after rehydration.** Each kit contains sufficient reagents for 96 wells and capable of assaying 40 duplicate samples.


ASSAY PROCEDURE

1. **Thoroughly read this protocol before performing an assay and please allow all kit components to return to room temperature before use(25-45 minutes).**
2. Dilute the **20x** assay buffer concentrate with 950ml of distilled water. This will be the **1x** assay buffer solution and used to dilute or dissolve all other reagents in this kit and samples.
Note: If crystals appear in the 20 assay buffer, the buffer can be placed in a warm water bath for approximately 30 minutes or until not crystal are visible. Mix thoroughly before use.
3. Centrifuge and dilute the standard peptide with 1ml of **1x** assay buffer, vortex. The concentration of this stock solution is 0.3µg/ml. Allow the solution to sit at least 10 minutes at room temperature (20-23°C) to completely dissolve in solution. Centrifuge and vortex immediately before use.

Prepare peptide standard solutions as follows:

Standard No.	Std. Volume	1x Assay Buffer	Concentrations
Stock	-----	1000µl	0.3µg/ml
#1	100µl of Stock	900µl	30ng/ml
#2	100µl of #1	900µl	3ng/ml
#3	100µl of #2	900µl	0.3ng/ml
#4	100µl of #3	900µl	0.03ng/ml

LEPTIN (MOUSE) EIA KIT PROTOCOL

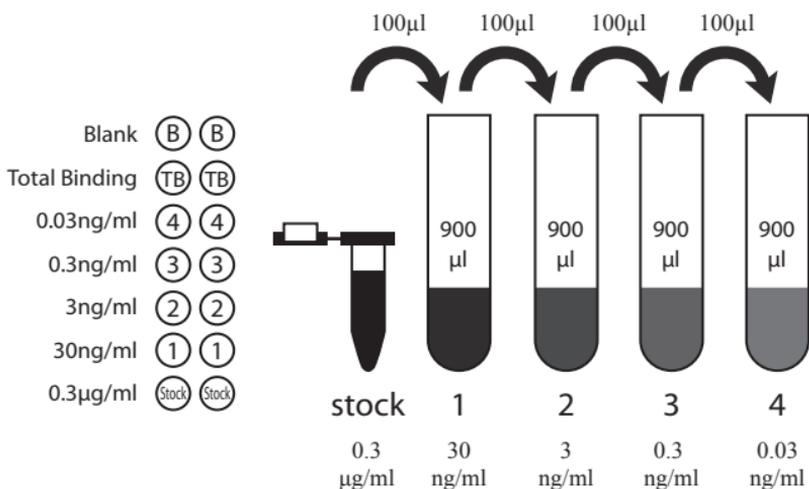

4. Remove immunoplate from the foil pouch and wash each well with 300µl of **1x** assay buffer. Allow it to sit for at least five minutes. Discard the buffer, invert and blot dry plate. Do not let wells dry before proceeding to the next step.
5. Centrifuge and rehydrate the positive control with 200µl of **1x** assay buffer. Allow the solution to sit at least 5 minutes to completely dissolve. Mix thoroughly.
6. Leave wells empty as **Blank**.
7. Add 50µl of **1x** assay buffer into wells B-1 and B-2 as Total Binding.
8. Add 50µl of prepared peptide standard from #4 to Stock (in reverse order of serial dilution into wells from C-1 to C-2 and G-1 to G-2 respectively.
Note: Peptide standards should be assayed in duplicate.
9. Add 50µl of rehydrated positive controls into wells H-1 and H-2.
Note: Positive controls should be assayed in duplicate.
10. Add 50µl of samples into their designated wells in duplicate.
11. Rehydrate the primary antibody (rabbit anti-peptide IgG) vial provided in this kit with 5ml of **1x** assay buffer. Allow it to sit for at least 5 minutes to completely dissolve. Mix thoroughly. Add 25µl of this solution into each well **except the Blank well**.

LEPTIN (MOUSE) EIA KIT PROTOCOL

12. Rehydrate the biotinylated peptide provided in this kit with 5ml of 1x assay buffer. Allow to sit for at least 5 minutes to completely dissolve. Mix thoroughly. Add 25 μ l of this solution into each well **except the Blank well**.
13. Seal the immunoplate with acetate plate sealer (APS). Incubate the immunoplate for 2 hours at room temperature (20-23C). Orbital shaking at 300-400rpm is recommended for the duration of the incubation.
14. Centrifuge the SA-HRP vial provided in this kit (3,000-5,000 rpm, 5 seconds) and pipette 12 μ l of SA-HRP into 12ml of 1x assay buffer to make SA-HRP solution, vortex thoroughly.
15. Remove APS from immunoplate. Discard contents of wells.
16. Wash each well with 350 μ l of 1x assay buffer, discard the buffer, invert and blot dry plate. Repeat 4 times.
17. Add 100 μ l SA-HRP solution into each well.
18. Reseal the immunoplate with APS. Incubate for 1 hour at room temperature (20-23°C). Orbital shaking at 300-400rpm is recommended for the duration of the incubation.
19. Remove APS from the immunoplate. Wash and blot dry the immunoplate 4 times with 1x assay buffer as described above in step 13.
20. Add 100 μ l of TMB substrate solution provided in this kit into each well. Orbital shaking at 300-400rpm is recommended for the duration of the incubation. After the addition of TMB solution, it is strongly recommended to cover the immunoplate to protect from light.
21. Reseal the immunoplate with APS. Incubate for 1 hour at room temperature (20-23°C).
22. Remove APS from the immunoplate. Add 100 μ l 2N HCl into each well to stop the reaction. The color in the well should change from blue to yellow. If the color change does not appear to be uniform, gently tap the plate to ensure thorough mixing. Go to the next step within 20 minutes.
23. Load the immunoplate onto a Microtiter Plate Reader. Read absorbance O.D. at 450nm.

ADDITIONAL RECOMMENDED PROCEDURAL NOTES:

- Reagents of different lot numbers should not be mixed.
- Recheck the reagent labels when loading the plate to ensure that everything is added correctly.
- Unused microplate strips should be placed in the foil pouch with a desiccant and stored at 4°C. Do not allow moisture to enter the wells.
- When handling the plate, avoid touching the bottom.
- Manual washing may cause high duplicate coefficient variations. To reduce this factor, liquid from the plate should be removed by inverting and blotting the plate on an absorbent material.
- If the room temperature is not within the suggested range (20-23°C), variations in results may occur.
- The same reservoir for the reagents may be reused if the reservoir is washed well with distilled water before each use.
- Each laboratory must determine the appropriate dilution factors for the samples to be measured to ensure that the samples are within the dynamic range of the standard curve.
- High levels of interfering proteins may cause variations within the sample results, therefore, it is imperative to select the appropriate sample preparation procedure to obtain the optimal results.
- Each time a new tip is used, make sure the tip is secure and free of air bubbles. For better intra-assay variation, aspirate and expel a reagent or sample back into the container a few times prior to loading.
- Avoid submerging the whole tip into reagents because droplets can accumulate at the end of the tip causing an excess of reagent to be loaded into the well. This can lead to poor results.
- For optimal results, an orbital plate shaker capable of 300-500 rpm is recommended for all incubations.
- Modification of the existing protocol (i.e. standard dilutions, pipetting technique, washing technique, incubation time or temperature, storage conditions, and kit expiration) may affect the sensitivity and specificity of the test.

CALCULATION OF RESULTS

Plot the standard curve on semi-log graph paper. A standard curve is constructed by plotting the known concentrations of standard peptide on the log scale (X-axis), and its corresponding O.D. reading on the linear scale (Y-axis). It is strongly recommended to use curve-fitting software capable of 4 parameter logistics or log-logit to quantify the concentration of standard peptide. The standard curve shows an inverse relationship between peptide concentrations and the corresponding O.D. absorbance. As the standard concentration increases, the intensity of the yellow color decreases, thereby reducing the O.D. absorbance.

The concentration of the peptide in a sample is determined by locating the sample's O.D. on the Y-axis, then drawing a horizontal line to intersect with the standard curve. A vertical line drawn from this point will intersect the X-axis at a coordinate corresponding to the peptide concentration in the sample. If samples have been diluted prior to the assay, the measured concentration must be multiplied by their respective dilution factors.

The standard curve will be a reverse sigmoidal shape.

Refer to the QC Data Sheet for acceptable values of the Positive Control.

STORAGE

1. Store the kit at 4°C upon receipt.
2. It is highly recommended that solution be used as soon as possible after rehydration.
3. Store 1x assay buffer at 4°C.
4. Remove any unneeded strips from Antibody-coated plate, re-seal them in zip-lock foil and keep at 4°C.
5. Keep rehydrated solution of Standard, Biotinylated peptide, Antibody, and HRP at 4°C. Prepare only the required amount.

SUMMARY OF ASSAY PROTOCOL

Add 50µl/well of standard, sample, or positive control, 25µl primary antibody, 25µl biotinylated peptide



Incubate at room temperature (20-23°C) for 2 hours



Wash immunoplate 4 times with 350µl/well of 1x assay buffer



Add 100µl/well of SA-HRP solution



Incubate at room temperature (20-23°C) for 1 hour



Wash immunoplate 4 times with 350µl/well of 1x assay buffer



Add 100µl/well of TMB substrate solution



Incubate at room temperature (20-23°C) for 1 hour



Terminate reaction with 100µl/well of 2N HCl




Read absorbance O.D. at **450nm** and calculate results.

REFERENCES

1. Portsmann, T., and Kiessig, S.T., Enzyme Immunoassay Techniques, An Overview, *Journal of Immunological Methods*, 150:5-21(1992).
2. Avrameas, S., Amplification Systems in Immunoenzymatic Techniques, *Journal of Immunological Methods*, 150: 23-32(1992).

ASSAY DIAGRAM

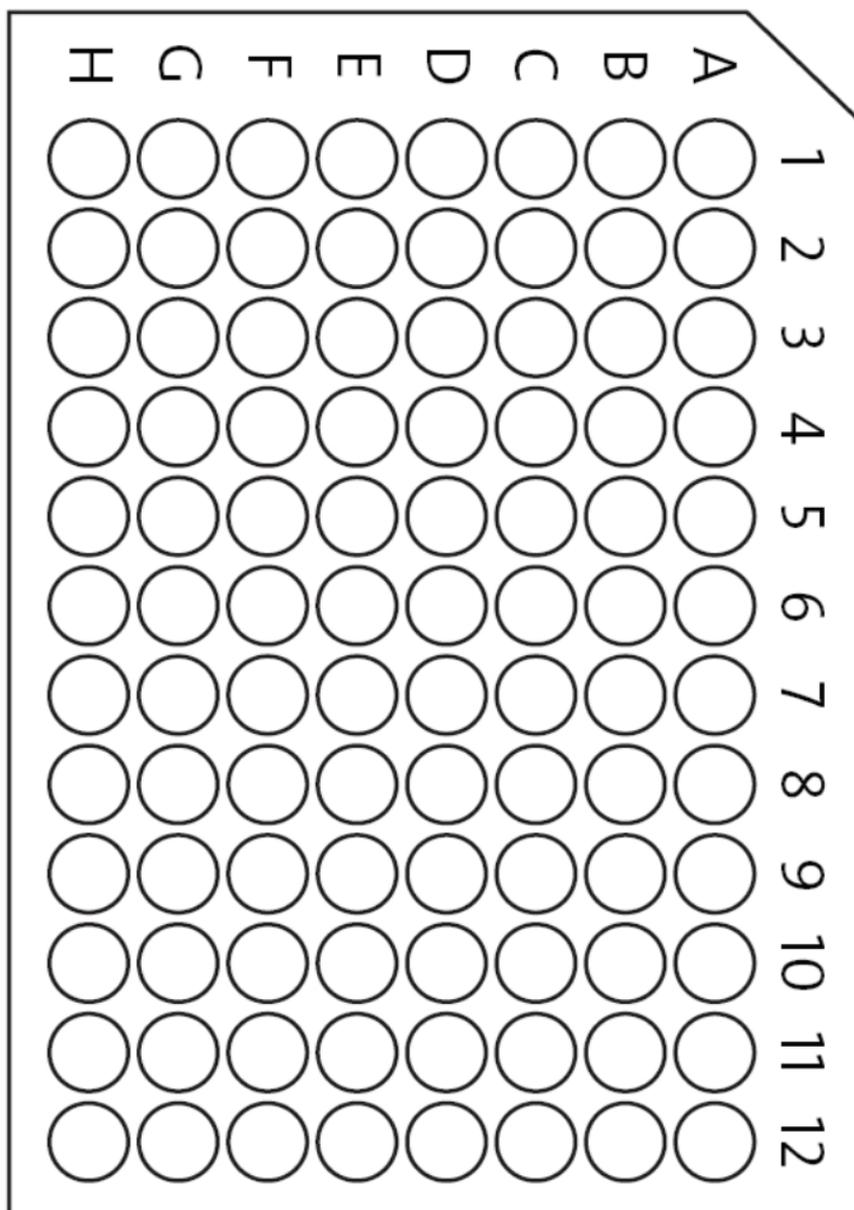

FOR RESEARCH ONLY

NOT FOR USE IN DIAGNOSTIC

PROCEDURES

USA

Phoenix Pharmaceuticals, Inc.

330 Beach Road, Burlingame,
California 94010
Tel: 650-558-8898, 800-988-1205
Fax: 650-558-1686
Info@PhoenixPeptide.com
www.Phoenix Peptide.com
12

Europe

Phoenix Europe GMBH

Viktoriastrasse 3-5
D-76133 Karlsruhe
Tel: +49(721) 1611950
Fax: +49(721)1611952
Germany@PhoenixPeptide.com